



FIELD OF ACTIVITY

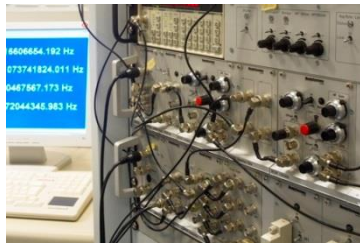

Practical realization of the definition of the metre



Practical realization of the definition of the radian



Surface texture: Roughness

The length laboratory is responsible for the development of the length and plane angles national metrology standards and as the following incumbencies:

- the realization of the practical definition of the metre and radian;
- calibrations;
- participation and coordination of interlaboratorial comparisons;
- technical support to the legal metrology.

SI UNIT

International System (SI) Base Unit of Length:

metre (m) defined as:

The length of the path travelled by light in a vacuum during a time interval of 1/299 792 458 of a second.

SI derived unit of the quantity Plane angle:

radian (rad) defined as:

The plane angle situated between two radius that, in a circumference of a circle, intersects an arc length equal to the radius of the mentioned circle.

TRACEABILITY

Length Quantity

At IPQ, the realization of the definition of the metre can be performed by two different ways:

1. By means of the wavelength in vacuum λ of a plane electromagnetic wave of frequency f ; this wavelength is obtained from the measured frequency f using the relation $\lambda = c_0 / f$ and the value of the speed of light in vacuum $c_0 = 299\,792\,458$ m/s.

The standard is an Optical Frequency Synthesizer (OFS) constituted by: an Nb:YVO₄ laser; an optical acoustic modulator, Kerr-lens mode-locked femtosecond Ti:sapphire laser and an optical fibre based on photonic crystals and an optical and electronic set that allows to determine the two frequencies that characterize the OFS, the offset frequency, f_0 , and the repetition frequency, f_r .

2. By means of one of the radiations included in the list recommended by BIPM, whose stated frequency wavelength in vacuum or whose stated frequency can be used with the uncertainty shown, provided that the given specifications and accepted good practice are followed.

The practical realization is based on the relation $c_0 = \lambda \times f$, and as the light speed, c_0 , is a constant and f (laser radiation frequency) is well determined, λ (wavelength) can be calculated.

In this case the standard is an He:Ne laser stabilized by molecular absorption in hyperfine iodine transition. Its traceability is obtained by the calibration with the OFS.

The use of this standards, or any other laser system calibrated by comparison with, allow the length measurements, ℓ , in terms of a number of wavelengths b , $\ell = \lambda \times b$, by interferometry.

TRACEABILITY



Plane Angle

The realization of the radian definition is made in terms of the circle subdivision. The complete circle corresponds to 2π rad. As π is an irrational number the units used in angular metrology belongs to the sexagesimal system and are the grade ($^{\circ}$), minute ($'$) and the second ($''$). As the sum of all intermediate angles of a circle is 360° and the sum of all errors of the same angles is zero, it is possible to produce matrixes and equations to determine the error of each intermediate angle of the circle. To make the practical realization of the radian definition, IPQ has an autocollimator (optical system used to measure small angular differences), an index table (allows the generation of angular positions) and gauge polygons. Nowadays, the traceability is reached through the calibration of the autocollimator at the international primary laboratory.



AVAILABLE SERVICES

Calibration

Length Domain

EQUIPMENT	RANGE	UNCERTAINTY	
Stabilized laser of the mise en pratique: vacuum wavelength/ absolute frequency	633 nm / 474 THz	$1 \times 10^{-8} \lambda_0$	
Other stabilized laser: vacuum wavelength	633 nm	1×10^{-11}	
Depth standard (ISO 5436-1 type A2): Parameter: depth d	0,1 μm to 10 μm	$(60 + 2d)$ nm d em μm	
Roughness standard (ISO 5436-1 type C): ISO roughness parameters: R_a R_z, R_p, R_v, R_t	0,1 μm to 10 μm 0,1 μm to 20 μm	$Q[50,30R_a]$ nm $Q[50,30R_z]$ nm	
Roughness standard (ISO 5436-1 type D): ISO roughness parameters: R_a R_z, R_p, R_v, R_t	0,1 μm to 10 μm 0,1 μm to 20 μm	$Q[50,30R_a]$ nm $Q[50,40R_z]$ nm	

Angle Domain

EQUIPMENT	RANGE	UNCERTAINTY	
Autocollimator	---	0,3''	
Angle block: included angle	0° to 90°	1,0''	
Optical polygon: face angle	4 to 24 faces		
Index table: index angle	$(0^{\circ}$ to $360^{\circ})$ step size: 30° , 40° or 60°		
Optical Square (pentaprism)	90°	0,5''	
Interferometer optical angular	N/A	0,50 μm	

$(L \text{ in mm}) Q[a, bL] = \sqrt{a^2 + (bL)^2}$

CONTACTS

INSTITUTO PORTUGUÊS DA QUALIDADE

(Portuguese Institute for Quality)

Rua António Gião, 2 , PT-2829-513 Caparica

LENGTH LABORATORY

Length, Angle
Head: Fernanda Saraiva, MSc
Tel: +351 212 948 160
E-mail: fsaraiva@ipq.pt

Mónica Fonseca, LSc
Tel: +351 212 948 183
E-mail: monicaf@ipq.pt